

QUALITY CONTROL CERTIFICATE

KIT NAME 88000-T4 HAZEL

| | | | |
|---------|----------|---------|---------|
| Code | 88000-T4 | | |
| Lot No. | 036 | 2025-05 | 2024-05 |

REAGENTS

| Label | Description | Lot. | Exp. | NO |
|-------|------------------------------|------|---------|-----|
| D6951 | 88000-T4 HAZEL | 036 | 2025-05 | 2X6 |
| B6950 | CALIBRATORE 88000-T4 HAZEL | 036 | 2025-06 | 1 |
| C6950 | CONTROL SERUM 88000-T4 HAZEL | 036 | 2025-06 | 1 |

CONTROLS

| | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

| | | |
|----------------------|------|----------|
| Calibrator (mOD) | 300 | ≥ 100 |
| Control Serum (KU/L) | 10,7 | 6,6-15,0 |

CALIBRATOR

| | | | | | | | | | | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 6 | 2 | 7 | 0 | 3 | 6 | 6 | 5 | 1 | 9 | 5 | 8 | 2 | 7 | 7 | 8 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES Operator Signature FB



CONTROL SERUM

| | | | | | | | | | | | | | | | | | |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 6 | 2 | 7 | 0 | 3 | 6 | 6 | 2 | 7 | 5 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES Operator Signature FB

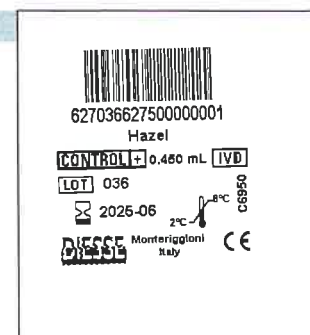

This batch has been manufactured and checked according to quality requirements. Hereby, it is released to distribution.

APPROVED RESPONSIBLE HEAD, Quality Control Reagents [Signature]

DATE 31/05/2024

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.