

QUALITY CONTROL CERTIFICATE

KIT NAME ANA-Screen - CHORUS

Code	86014		
Lot No.	943	2024-06	2023-06

REAGENTS

Label	Description	Lot.	Exp.	NO
D3141	ANA-Screen	943	2024-06	6X6
B3141	CALIBRATORE ANA-Screen	943	2024-06	1
C3141	CONTROL SERUM ANA-Screen	943	2024-06	1

CONTROLS


	Found results	Expected results
--	---------------	------------------

Calibrator (mOD)	339	> 100
Control Serum (Ndx)	3,5	2,3-4,3

CALIBRATOR

1	1	5	9	4	3	6	0	0	0	0	0	3	0	0	0	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader YES  Operator Signature *Blum*

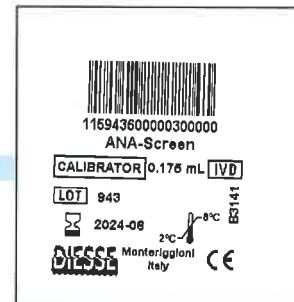

CONTROL SERUM

1	1	5	9	4	3	6	2	3	4	3	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader YES  Operator Signature *Blum*



*This batch has been manufactured and checked according to quality requirements. Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents..... *Blum*

DATE *24-06-2023*

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.