

DIESSE DIAGNOSTICA SENESE SpA
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

QUALITY CONTROL CERTIFICATE

KIT NAME U1-70 RNP - CHORUS

Code 86088

Lot No. 964



2024-08



2023-09

REAGENTS

Label	Description	Lot.	Exp.	NO
D3662	U1-70 RNP	964	2024-08	6X6
B3662	CALIBRATORE U1-70 RNP	964	2024-08	1
C3662	CONTROL SERUM U1-70 RNP	964	2024-08	1

CONTROLS

	Found results	Expected results
--	---------------	------------------

Calibrator (mOD)	494	≥ 100
Control Serum (AU/mL)	41,5	39,2-114,3

CALIBRATOR

1	0	4	9	6	4	6	3	2	3	3	4	4	0	4	8	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES



Operator Signature



CONTROL SERUM


1	0	4	9	6	4	6	1	9	3	5	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES



Operator Signature

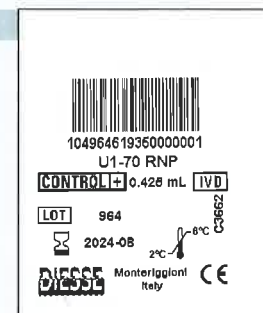

*This batch has been manufactured and checked according to quality requirements.
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

DATE 15.09.2023

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.

DIESSE DIAGNOSTICA SENESE SpA
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

QUALITY CONTROL CERTIFICATE

KIT NAME U1-70 RNP - CHORUS

Code 86088

Lot No. 964



2024-08



2023-09

REAGENTS

Label	Description	Lot.	Exp.	NO
D3662	U1-70 RNP	964	2024-08	6X6
B3662	CALIBRATORE U1-70 RNP	964	2024-08	1
C3662	CONTROL SERUM U1-70 RNP	964	2024-08	1

CONTROLS

	Found results	Expected results
--	---------------	------------------

Calibrator (mOD)	494	≥ 100
Control Serum (AU/mL)	41,5	39,2-114,3

CALIBRATOR


1	0	4	9	6	4	6	3	2	3	3	4	4	0	4	8	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES



Operator Signature

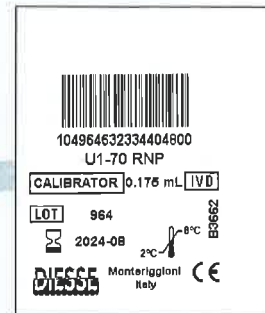

CONTROL SERUM


1	0	4	9	6	4	6	1	9	3	5	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES



Operator Signature

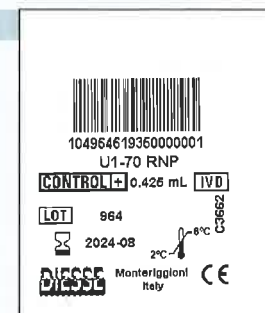

*This batch has been manufactured and checked according to quality requirements.
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

DATE 15.09.2023

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.