



DIESSSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020

Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

**QUALITY CONTROL CERTIFICATE**

**KIT NAME** SYPHILIS SCREEN RECOMBINANT - CHORUS

Code	81100		
Lot No.	970	2024-09	2023-09

**REAGENTS**

Label	Description	Lot.	Exp.	NO
D2541	Syphilis Screen Recombinant	970	2024-09	6X6
B2541	CALIBRATORE Syphilis Screen Recombinant	970	2024-09	1
C2541	CONTROL SERUM Syphilis Screen Recombinant	970	2024-09	1


**CONTROLS**

	Found results	Expected results
Calibrator (mOD)	480	≥ 100
Control Serum (INDEX)	2,1	1,5-2,8
Negative Control (INDEX)	0,1	<0,7

**CALIBRATOR**

0	3	2	9	7	0	6	0	0	0	0	0	0	4	6	0	0	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---


Label checked with barcode reader YES  Operator Signature



**CONTROL SERUM**

0	3	2	9	7	0	6	1	5	2	8	0	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader YES  Operator Signature

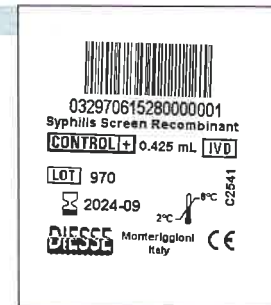

*This batch has been manufactured and checked according to quality requirements. Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

DATE 06/10/2023

**WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!**

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.