

DIESE DIAGNOSTICA SENESE SpA
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39
Tel. +39 0577319554



QUALITY CONTROL CERTIFICATE

KIT NAME CHLAMYDOPHILA PNEUMONIAE IgA - CHORUS

Code	81252		
Lot No.	026	2025-04	2024-04

REAGENTS

Label	Description	Lot.	Exp.	NO
D8610	Chlamydomphila pneumoniae IgA	026	2025-04	6X6
B8610	CALIBRATORE Chlamydomphila p. IgA	026	2025-04	1
C8610	CONTROL SERUM Chlamydomphila p. IgA	026	2025-04	1

CONTROLS


	Found results	Expected results
--	---------------	------------------

Calibrator (mOD)	520	≥ 100
Control Serum (AU/mL)	34,4	21,8-43,5
Negative Control (AU/mL)	<10,0	≤ 10,0

CALIBRATOR

1	9	9	0	2	6	6	8	1	2	2	3	5	5	4	0	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---


Label checked with barcode reader YES Operator Signature FB



CONTROL SERUM

1	9	9	0	2	6	6	1	3	2	4	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader YES Operator Signature FB

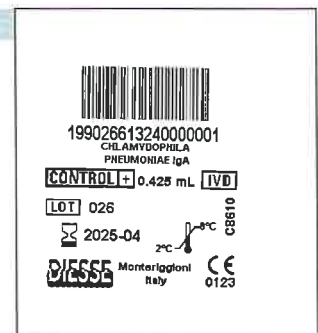

This batch has been manufactured and checked according to quality requirements. Hereby, it is released to distribution.

APPROVED RESPONSIBLE HEAD, Quality Control Reagents..... FB

DATE 26/06/2024

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.